



# Ultrasonic Bone Surgery System VarioSurg 4

# **Control panel**

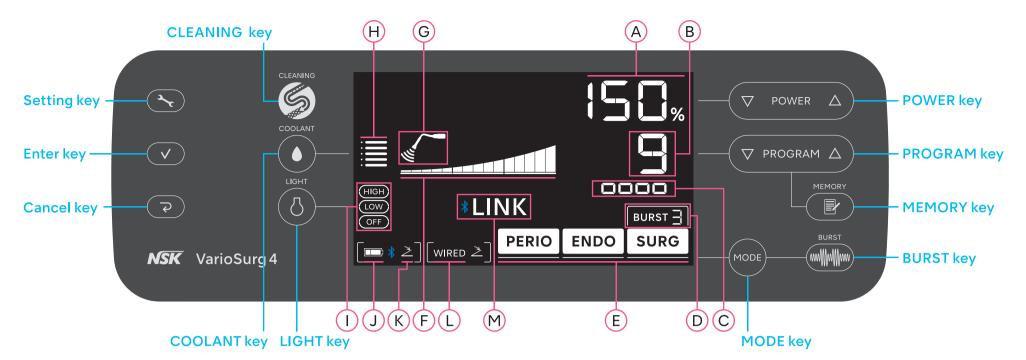


#### **Foot control**

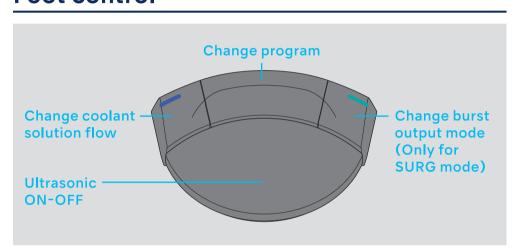

Α	Power level							
В	Program No.							
С	Status of wireless foot control calibration successful							
D	Burst output level							
Е	Mode							
F	Power level is indicated by the number of indicator bars.							
G	Vibration							
Н	Coolant solution flow level							


1	Light level
J	Battery level of the wireless foot control
K	Status of connection with the wireless foot control
L	Status of connection with the wired foot control
Μ	Status of connection with the Surgic Pro2

## **Preparation for Use**

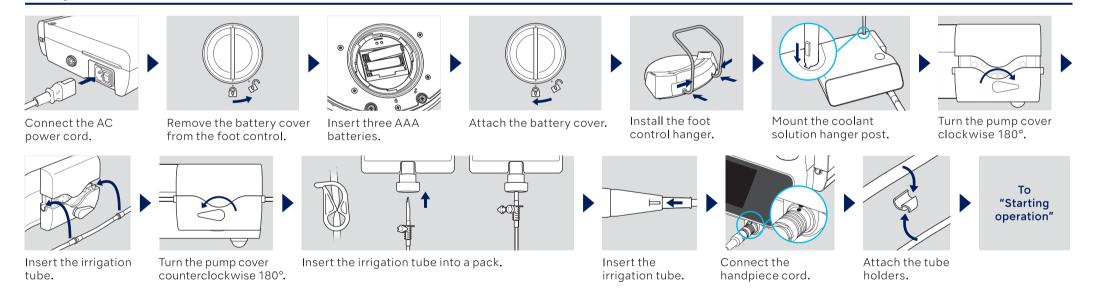

#### Starting operation

Surgic Pro2.

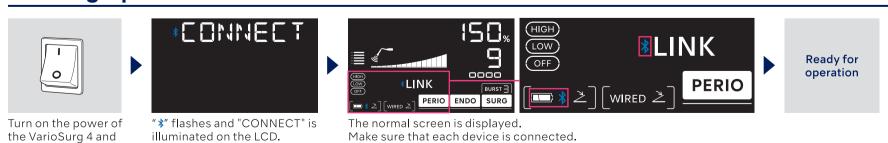

## **Link with Surgic Pro2**

## Step 1. VarioSurg 4



Press and hold the Setting key. "BLE SET" is displayed.



Press the Enter key.



Press the PROGRAM key to select "LK".




"LK" and "LINK" flash.



Press the Enter key.
"PAIRING" and "LK" are illuminated.

\*and "LINK" flash.


## Step 2. Surgic Pro2



Press and hold the Setting key. "BLE SET" is displayed.




Press the Enter key.



Press the TORQUE key to select "LK".



"LK" and "VARIOSURG" flash.




Press the Enter key.
"PAIRING" and "LK" are illuminated.

\*and "VARIOSURG" flash.

#### Step 3. VarioSurg 4 / Surgic Pro2

#### VarioSurg 4



Pairing is successful when this product beeps and device displays "OK". Make sure ≯ is displayed and the device is connected.

×2


Press the Cancel key to return to the normal screen.

#### Surgic Pro2



Pairing is successful when this product beeps and device displays "OK".

Make sure \* is displayed and the device is connected.



Press the Cancel key to return to the normal screen.

# **VarioSurg Tips MODE & POWER GUIDE**

Model	Mode	Max	Model	Mode	Max	Model	Mode	Max	Model	Mode	Max	Model	Mode	Max
H-SG1	S	150%	SG5	S	80%	SG18R	S	50%	SCL1	S	50%	E32D-S	Е	50%
H-SG8	S	150%	SG6D	S	80%	SG18L	S	50%	SCL1D	S	80%	G1-S	S	50%
H-SG8R	S	150%	SG7D	S	50%	SG19	S	80%	SCL2D	S	80%	P20-S	P	100%
H-SG8L	S	150%	SG8	S	80%	SG30	S	50%	SCL3	S	50%	P25R-S	Р	100%
SG58	S	80%	SG8A	S	80%	SG15A	S	50%	SCL3D	S	80%	P25L-S	Р	100%
SG1	S	80%	SG9	S	50%	SG15B	S	50%	SCL4D	S	80%	V-P10	Р	100%
SG1A	S	80%	SG10	S	50%	SG15C	S	50%	SCL5	S	50%	V-P11R	Р	100% *
SG2R	S	80%	SG11	S	50%	SG15D	S	50%	SCL5D	S	80%	V-P11L	Р	100% *
SG2L	S	80%	SG14R	S	80%	SG16A	S	50%	E30RD-S	Е	50%	V-P12	Р	100% *
SG3	S	80%	SG14L	S	80%	SG16B	S	50%	E30LD-S	E	50%	Warning: To be used only with VarioSurg 3 and VarioSurg 4.		
SG4	S	80%	SG17	S	80%	SG68	S	80%	E31D-S	E	50%			
									<u> </u>			_		